



Direct Saliva MELATONIN

ELISA

This product is for research use only
It is not intended for use in diagnostic procedures

EK-DSM-U 96 tests

Revision date: 2012-12-14

ENGLISH

INTENDED USE

The BÜHLMANN Direct Saliva Melatonin ELISA (EK-DSM-U) is intended for highly sensitive, quantitative determination of melatonin in human saliva (1-4). This product is for research use only. It is not intended for use in diagnostic procedures.

PRINCIPLE OF THE ASSAY

The BÜHLMANN Direct Saliva Melatonin ELISA is a competitive immunoassay using a capture antibody (Ab) technique. The polyclonal Kennaway G280 anti-melatonin antibody (5,6) has been coated onto the microtiter plate, provided in the kit. After the first 16-20 hours over night incubation, melatonin present in the pre-treated saliva and controls as well as in the calibrators, compete with biotinylated melatonin during a 3 hours incubation for the binding sites of this highly specific antibody. After washing, the enzyme label, streptavidin conjugated to horseradish peroxidase (HRP) is added, which binds during a third 60 minutes incubation step to the melatonin-biotin-antibody complexes captured on the coated wells. Unbound enzyme label is then removed by a second washing step and TMB substrate (tetramethylbenzidine) is added to the wells. In a fourth 30 minutes incubation step, a chromophore is formed in inverse proportion to the amount of melatonin present in the sample. The color turns from blue to yellow after the addition of an acidic stop solution and can be measured at 450 nm.

REAGENTS SUPPLIED AND PREPARATION

| Reagents | Quantities | Code | Reconstitution |
|---|--------------------|----------------|---|
| Pretreatment Solution | 1 vial 5 ml | B-EKDSM-PRS | Ready to use corrosive |
| Neutralizing Solution | 1 vial 5 ml | B-EKDSM-NS | Ready to use irritant |
| Microtiter Plate precoated with G280 anti-melatonin Ab | 12x8 wells | B-EKDSM-MP | Wash 2x before use |
| Plate Sealer | 3 pieces | | |
| Wash Buffer Concentrate (10x) with preservatives | 1 bottle 100 ml | B-EKDSM-WB | Dilute with 900 ml deionized water |
| Blanking Reagent¹⁾ lyophilized | 1 vial 1 ml | B-EKDSM-BR | Dissolve in 1ml Incubation Buffer |
| Incubation Buffer (Zero Calibrator) melatonin-free buffer | 1 vial 12 ml | B-EKDSM-IB | Ready to use |
| Calibrators²⁾ lyophilized; do not pretreat | 5 vials lyoph. | B-EKDSM-CASET | Reconstitute with 1ml Incubation Buffer |
| Control low / high³⁾ for pretreatment see page 3 | 2 vials lyophl | B-EKDSM-CONSET | Reconstitute with 1ml Incubation Buffer |
| Biotin Conjugate | 1 vial 5.5 ml | B-EKDSM-BC | Ready to use |
| Enzyme Label Streptavidin conjugated to HRP | 1 vial 11 ml | B-EKDSM-EL | Ready to use |
| TMB Substrate buffered with citrate and H ₂ O ₂ | 1 vial 11 ml | B-TMB | Ready to use |
| Stop Solution 0.25 M sulfuric acid | 1 vial 11 ml | B-ST5 | Ready to use |

Table 1

¹⁾ The Blanking reagent contains a saturated melatonin solution. Prevent any contamination of other kit reagents.

²⁾ The Calibrators A, B, C, D and E contain the following melatonin concentration: 0.48, 1.2, 3.2, 8.0 and 20 pg/ml which are corrected for the 20% sample dilution during pretreatment and therefore, labeled with 0.6, 1.5, 4.0, 10, and 25 pg/ml of melatonin, respectively.

³⁾ Lot specific amount of melatonin see data sheet added to the kit.

STORAGE AND SHELF LIFE OF REAGENTS

| Unopened Reagents | |
|--|---|
| Store at 2-8°C until expiration date. Do not use past expiration date. | |
| Opened / Reconstituted Reagents | |
| Microtiter Plate | Return unused strips immediately to the plastic pouch containing the desiccant pack and reseal along the entire edge of zip-seal. Store for up to 2 months at 2-8°C |
| Pretreatment Reagent | Store at 2-8°C until expiration date printed on the labels. |
| Neutralizing Solution | |
| Incubation Buffer | |
| Wash Buffer diluted | Store at 2-8°C up to 6 months |
| Blanking Reagent | Stable at 2-8°C up to 4 months. |
| Calibrators | |
| Controls | |
| Biotin Conjugate | Store at 2-8°C until expiration date printed on the labels. |
| Enzyme Label | |
| TMB Substrate | |
| Stop Solution | |

Table 2

WARNINGS AND PRECAUTIONS

The Microtiter Plate (B-EKDSM-MP) contains components of human origin. Each serum donor unit used in the preparation of the kit components was tested by an FDA approved method and found negative for HBV surface antigen, so as for HCV and HIV1/2 antibodies. Although these methods are highly accurate, there is no guarantee that this material cannot transmit Hepatitis or AIDS. Therefore, all samples and kit components should be handled as if capable of transmitting infections. All products containing human source material should be handled in accordance with appropriate precautions. Disposal of any discarded materials should be in accordance to local requirements.

Pretreatment/Neutralizing Solution: The Pretreatment Solution (B-EKDSM-PRS) contains sodium hydroxide (NaOH) and the Neutralizing solution (B-EKDSM-NS) contains hydrochloric acid (HCl). The reagents are irritants to eyes, skin and mucous membranes. Avoid contact with eyes, skin and clothing. Wear suitable protective clothing, gloves and eye protection. After contact with eyes or skin, wash immediately with plenty of water (cf. MSDS).

MATERIALS REQUIRED BUT NOT PROVIDED

- Precision pipettes with disposable tips: 5, 50, 100 µl and 1 ml pipettes. Repeater or multichannel pipette for 50 and 100 µl.
- Disposable polystyrene or polypropylene tubes for the preparation of sample dilutions.
- 1000 ml cylinder for dilution of the Wash Buffer.
- Microtiter plate washer or squeeze bottle for Wash Buffer.
- Blotting paper.
- Refrigerator.
- Microtiter plate rotator.
- Microtiter plate reader for measurement of absorbance at 450 nm.
- BÜHLMANN Saliva Collection Devices, B-SLEEPCHECK16 or B-SVC/5.

PROCEDURAL NOTES FOR SAMPLE COLLECTION

Collect saliva using the BÜHLMANN Saliva Collection Devices. The devices can absorb up to 3 ml of saliva. The procedure calls for 0.2 ml of saliva.

Saliva collection is simple and can be performed in s' home at his convenience, but following precautions are recommended:

Please read the instructions carefully before starting to collect saliva. The more carefully you follow the instructions, the more reliable the results will be.

Individuals should set aside an evening for this test avoiding sporting activities and any intense efforts as far as possible.

Light: Bright light can suppress melatonin production. Therefore, it is important to avoid bright light during the test. Muted lighting from a reading lamp or from the television is preferable.

Eating: Nothing should be eaten during the collection time. The last meal must be taken at least 30 minutes before starting the collection. Bananas and chocolate should not be eaten during the entire day before the collection.

Drinking: Drinks containing artificial colorants, caffeine (coffee, black or green tea, iced tea, cola) or alcohol are not allowed on the evening of the collection.

Medicines: On the collection day, if possible, no aspirin and medicines that contain ibuprofen (Algiofor, Brufen, Dysmenol, Dolocyl, Ecopropfen) should be taken. If your sleep or sleep-wake rhythm is treated with melatonin, this must be discontinued at least one week before the collection.

SAMPLE SHIPMENT AND STORAGE

Shipment: The collected saliva samples (Salivette® tubes) must be shipped to the laboratory within two days. Used salivette tubes must be kept in the fridge at 2-8°C. Samples should not be sent on Fridays, Saturdays or the day before holiday.

Storage: The saliva samples absorbed in the cotton swab may be stored in the saliva collection device for up to 7 days at 2-8°C. If not assayed within one week after collection, samples should be frozen and may be stored for at least 6 months at ≤ -20°C. Repeated freeze-thaw cycles should be avoided.

PROCEDURAL NOTES

The blanking reagent contains a saturated melatonin solution. Avoid any contamination of other reagents of this kit. Change disposable tips after each pipetting step.

The assay procedure has been optimized for Sleep Check application. Therefore Blank reagent and Calibrators are assayed in duplicates, whereas controls and samples are measured in single determinations. This approach allows you to test 16 individual profiles (5 points) per microtiter plate. For applications other than Sleep Check duplicate determinations are recommended.

SAMPLE COLLECTION



1 Before starting collection, label the tubes. Add name, date of birth, collection date and time.



2 15 minutes before each saliva sample, rinse your mouth thoroughly with water.



3 Open the top of the tube (the swap is in the top) and remove the top from the tube.



4 Put the swap into your mouth straight from the top without touching it with your fingers.



5 Put the swap between your teeth and cheek and move it around with your tongue for 3-5 minutes, until the swap is thoroughly soaked with saliva.



6 Put the swap from your mouth straight into the tube, without touching it with your fingers.



7 Using the top, push the swap into the tube and put on the top. For the collection of a melatonin profile repeat step 1 to 7 as indicated.

Store the samples refrigerated at 2-8°C.

SAMPLE PRETREATMENT (LABORATORY)

Sample recovery from Salivette®

Centrifuge the Salivette® tubes sent by the for around 5 min at 3000 rpm (~1500x g). Discard the suspended insert with the swap and store the tube at 2-8°C or -20°C.

Pretreatment of Saliva Samples and Controls

- Pipet 200 µl of controls and saliva samples, respectively, into correspondingly marked, clean polypropylene, tubes.
- Add 25 µl of pretreatment solution to each tube using a multipipettor device.
- Vortex for 5 seconds and leave the tubes for 10 minutes at 18-28°C.
- Add 25 µl of neutralizing solution to each tube using a multipipettor device. Vortex for 5 seconds.
- Centrifuge the pre-treated samples for 5 min at 10'000 rpm. Proceed to the ELISA procedure.

ASSAY PROCEDURE

1. Use a plate with enough 8-well strips to test the desired number of Blanks, Calibrators, Controls and samples. Remove excess strips from the holder and re-seal them in the plastic bag together with the two desiccant bags **without delay**. Store refrigerated.
2. Wash the coated strips twice using at least 300 µl of Wash Buffer per well. Empty the wells and strike the plate firmly onto blotting paper.
- 3a. Pipet 100 µl of Blanking Reagent (Blank) in duplicate into wells A1+A2.

- 3b. Pipet 100 µl of Incubation Buffer (Zero Calibrator) in duplicate into wells B1+B2.
 - 3c. Pipet 100 µl of Calibrator A in duplicate into wells C1+ C2
Pipet 100 µl of Calibrator B in duplicate into wells D1+D2
Pipet 100 µl of Calibrator C in duplicate into wells E1+E2
Pipet 100 µl of Calibrator D in duplicate into wells F1+F2
Pipet 100 µl of Calibrator E in duplicate into wells G1+G2
 - 3d. Pipet 100 µl of pretreated Low Control (single) into well H1
Pipet 100 µl of pretreated High Control (single) into well H2
 - 3e. Pipet 100 µl of each pretreated sample (single) into the subsequent wells.
 4. Cover the plate with a plate sealer and incubate for 16-20 hours **at 2-8°C**.
 5. Remove and discard the plate sealer. Add 50 µl of Biotin Conjugate (blue solution) to each well. Cover the plate with a plate sealer and place it for 1 min on a plate rotator set at 600 rpm.
 6. Incubate for 3 hours (± 5 minutes) **at 2-8°C**.
 7. Remove and discard the plate sealer. Aspirate or invert the plate to empty the solution from each well and wash four times using at least 300 µl of wash buffer per well. Empty the wells and strike the plate firmly onto blotting paper.
 8. Add 100 µl of Enzyme Label (yellow solution) to all wells.
 9. Cover the plate with a new plate sealer, place the plate on a plate rotator set at 600 rpm and incubate for 60 minutes (± 5 minutes) at 18-28°C.
 10. Remove and discard the plate sealer. Aspirate or invert the plate to empty the solution from each well and wash four times using at least 300 µl of wash buffer per well. Empty the wells and strike the plate firmly onto blotting paper.
- Important:** allow the TMB Substrate to come to 18-28°C prior to use.
11. Add 100 µl of TMB Substrate to all wells.
 12. Cover the plate, place it on a plate rotator set at 600 rpm, protect the plate from direct light and incubate for 30 \pm 5 minutes at 18-28°C.
 13. Add 100 µl of Stop Solution to all wells. Remove air bubbles by pricking them with a pipette tip. Proceed to step 14 within 30 minutes.
 14. Read the absorbance at 450 nm in a microtiter plate reader.

RESULTS

Standard Curve: Record the absorbance at 450 nm for each calibrator, Incubation Buffer and Blank well. Average the duplicate values, subtract the average of the Blank wells and record averages (=corrected average absorbance). Calculate the binding (B) of each pair of calibrator wells as a percent of Incubation Buffer (B_0), with the Blank-corrected absorbance of the Incubation Buffer taken as 100 %.

$$B / B_0 (\%) = \text{percent bound} = \frac{\text{net absorbance}}{\text{net absorbance of Zero Calibrator}} \times 100$$

Plot the percent bound (vertical axis) versus the concentration of melatonin in pg/ml (horizontal axis) using a lin/log graph paper. Draw the best fitting curve or calculate the standard curve using a four parameter algorithm.

Samples and Controls: Record the absorbance at 450 nm for each sample well. Subtract the average of the blank wells and record the absorbance (=corrected average absorbance). Calculate, as described above, the binding of each pair of sample wells as a percent of Incubation Buffer

(B_0), with the Blank-corrected absorbance of Incubation Buffer taken as 100%. Locate the B/B_0 value of the samples on the vertical axis, draw a horizontal line intersecting the standard curve and read the melatonin concentration (pg/ml) from the horizontal axis.

See Table 3 and Figure 1 for examples of results and standard curves. *These results and standard curves are for demonstration purposes only. A standard curve must be generated for each set of samples to be assayed.*

PERFORMANCE CHARACTERISTICS

Intra-Assay Precision (Within-Run): 12.6%. The intra-assay precision was calculated from the results of four different saliva samples within the standard range, measured 10 times in duplicate in a single run. The results are presented in Table 4.

Inter-Assay Precision (Run-to-Run): 22.9%. The inter-assay precision was calculated from the results of 17 independent runs with 5 samples within the standard range. The results are presented in Table 5.

Dilution Linearity/Parallelism: 92.2%. Three saliva samples with high amount of melatonin were sequentially diluted with Incubation Buffer and assayed according to the assay procedure. The Results are presented in Table 6. Due to the complex matrix of saliva samples dilution with Incubation Buffer higher than 1:8 will cause a decreased linearity. Therefore sample dilution with Incubation Buffer higher than 1:4 is not recommended.

Spiking Recovery: 97.9%. Two saliva samples from the same donor, one collected during daytime and one during night time were titrated against each other and assayed according the assay procedure twice, independently. The Results are presented in Table 7.

Due to the complex and individual nature of the saliva matrix direct spiking of saliva with melatonin can lead to decreased recovery rates.

Analytical Sensitivity (Limit of Detection – LOD): 0.5 pg/ml. 32 wells of Incubation Buffer (Zero Calibrator) were assayed in two independent runs. The minimum detectable concentration in 0.1 ml of Incubation Buffer was calculated by subtracting two standard deviations of averaged Refer values from the OD of Zero calibrator and intersecting the value with the standard curve obtained in the same run.

Functional Sensitivity (Limit of Quantification – LOQ): 1.6 – 20.5 pg/ml. The limit of quantification of this assay is the melatonin concentration in saliva that can be measured with an inter-assay coefficient of variation (CV) of less than 30%. The LOQ was determined from 7 different samples from 1.3 – 47.3 pg/ml each sample measured 17 times in duplicate in independent runs.

Specificity: the 50% binding (cross-reactivity) of the melatonin antiserum with different compounds were tested in the Direct Saliva Melatonin Radioimmunoassay (RK-DSM) from BÜHLMANN AG and are presented in Table 8.

METHOD COMPARISON

The comparison was done with 78 saliva samples from 10 different donors collected at different daytimes. The samples were analyzed using the presented EK-DSM-U assay as well as the Direct Saliva Melatonin Radioimmunoassay (RK-DSM) from BÜHLMANN AG. The subsequent linear regression analysis resulted in a correlation factor of $R^2 = 0.84$, an intercept of 0.77 pg/ml and a slope of 1.21. The correlation is presented in Figure 3.

Table 3: **Example of Results**

| | Conc. (pg/ml) | Absorbance (OD) | B/B0 (%) | CV Conc. (%) | Calc. Conc. (pg/ml) |
|-----------------|---------------|-----------------|--------------|--------------|---------------------|
| Blank | | 0.075 | | | |
| Blank | | 0.067 | | 5.6 | |
| Avg. | | 0.071 | | | |
| Zero Calibrator | | 1.715 | 98.5 | | |
| Zero Calibrator | 0.0 | 1.766 | 101.5 | 2.1 | |
| Avg. | | 1.741 | 100.0 | | |
| Cal A | | 1.484 | 85.3 | | |
| Cal A | 0.6 | 1.514 | 87.0 | 1.4 | |
| Avg. | | 1.499 | 86.1 | | |
| Cal B | | 1.292 | 74.2 | | |
| Cal B | 1.5 | 1.274 | 73.2 | 1.0 | |
| Avg. | | 1.283 | 73.7 | | |
| Cal C | | 0.755 | 43.4 | | |
| Cal C | 4.0 | 0.769 | 44.2 | 1.3 | |
| Avg. | | 0.762 | 43.8 | | |
| Cal D | | 0.364 | 20.9 | | |
| Cal D | 10 | 0.359 | 20.6 | 1.0 | |
| Avg. | | 0.362 | 20.8 | | |
| Cal E | | 0.179 | 10.3 | | |
| Cal E | 25 | 0.182 | 10.5 | 1.2 | |
| Avg. | | 0.181 | 10.4 | | |
| Ctrl. high | | 0.560 | 32.2 | | 6.2 |
| Ctrl. high | | 0.553 | 31.8 | 0.9 | 6.3 |
| Avg. | | 0.557 | 32.0 | | 6.2 |
| Ctrl. low | | 0.929 | 53.4 | | 2.9 |
| Ctrl. low | | 0.874 | 50.2 | 4.3 | 3.3 |
| Avg. | | 0.902 | 51.8 | | 3.1 |
| Sample 01 | | 0.414 | 23.8 | | 8.9 |
| Sample 01 | | 0.404 | 23.2 | 1.7 | 9.2 |
| Avg. | | 0.409 | 23.5 | | 9.0 |
| Sample 02 | | 0.970 | 55.7 | | 2.7 |
| Sample 02 | | 0.908 | 52.2 | 4.7 | 3.0 |
| Avg. | | 0.939 | 54.0 | | 2.9 |
| Sample 03 | | 1.215 | 69.8 | | 1.6 |
| Sample 03 | | 1.162 | 66.8 | 3.2 | 1.8 |
| Avg. | | 1.189 | 68.3 | | 1.7 |

ED20 = 10.9 pg/ml ED50 = 3.3 pg/ml ED80 = 1.0 pg/ml

Figure 1: **Example of Standard Curve**

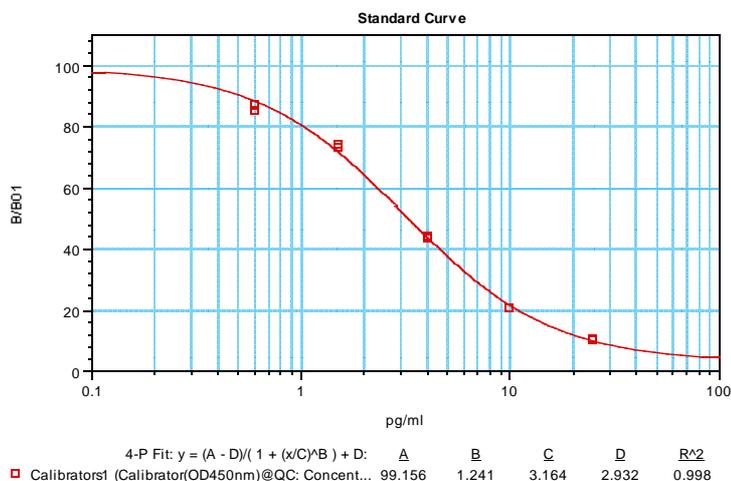


Figure 2: **Pipetting Scheme**

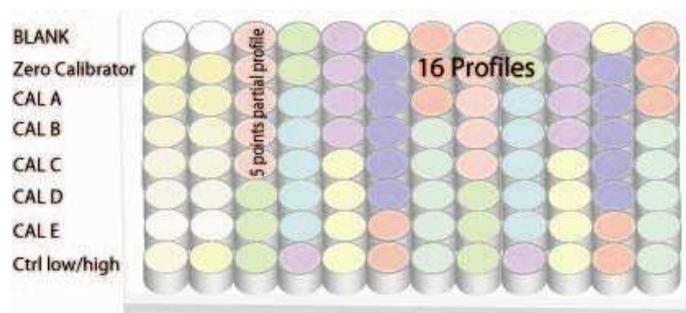


Table 4: **Intra-Assay Precision**

| Sample | Mean [pg/ml] | SD [pg/ml] | CV [%] |
|--------|--------------|------------|--------|
| S01 | 1.7 | 0.19 | 11.2 |
| S04 | 5.2 | 1.20 | 22.9 |
| S03 | 13.7 | 1.48 | 10.8 |
| S05 | 15.9 | 0.84 | 5.3 |
| Mean | | | 12.6 |

Table 5: **Inter-Assay Precision**

| Sample | Mean [pg/ml] | SD [pg/ml] | CV [%] |
|-----------|--------------|------------|--------|
| Ctrl low | 2.6 | 0.59 | 23.8 |
| S11 | 2.4 | 0.41 | 17.2 |
| S12 | 4.6 | 1.32 | 28.8 |
| Ctrl high | 5.2 | 1.20 | 23.2 |
| S13 | 13.7 | 3.05 | 22.3 |
| Mean | | | 22.9 |

Table 6: **Dilution Linearity/Parallelism**

| Sample | Dilution Factor | Observed [pg/ml] | Expected [pg/ml] | Recovery O/E [%] |
|--------|-----------------|------------------|------------------|------------------|
| S06 | 1:1 | 14.9 | -- | -- |
| | 1:2 | 7.8 | 7.5 | 104.7 |
| | 1:4 | 3.0 | 3.7 | 80.5 |
| | [1:8] | [1.1] | [1.9] | [59.1] |
| S07 | 1:1 | 22.7 | -- | -- |
| | 1:2 | 11.6 | 11.4 | 102.2 |
| | 1:4 | 5.0 | 5.7 | 88.1 |
| | [1:8] | [1.8] | [2.8] | [63.4] |
| S08 | 1:1 | 20.4 | -- | -- |
| | 1:2 | 13.1 | 13.6 | 96.3 |
| | 1:4 | 6.4 | 6.8 | 94.1 |
| | [1:8] | [2.7] | [3.4] | [79.4] |
| Mean | | | | 92.2 |

Table 7: Spiking Recovery

| Sample | Titration Ratio S5/S8 | Expected [pg/ml] | Observed [pg/ml] | Recovery O/E [%] |
|--------|-----------------------|------------------|------------------|------------------|
| S5/S8 | 5/0 | 1.2 | 1.2 | -- |
| | 4/1 | 4.3 | 4.4 | 102.8 |
| | 3/2 | 7.4 | 5.3 | 72.0 |
| | 2/3 | 10.4 | 9.8 | 93.9 |
| | 1/4 | 13.5 | 13.9 | 102.8 |
| | 0/5 | 16.6 | 16.6 | -- |
| S5/S8 | 5/0 | 0.9 | 0.9 | -- |
| | 4/1 | 3.7 | 3.6 | 96.8 |
| | 3/2 | 6.5 | 6.4 | 97.9 |
| | 2/3 | 9.4 | 10.5 | 112.2 |
| | 1/4 | 12.2 | 12.8 | 105.1 |
| | 0/5 | 15.0 | 15.0 | -- |
| Mean | | | | 97.9 |

Table 8 Specificity

| Compound | Crossreactivity [%] |
|------------------------------|---------------------|
| melatonin | 100 |
| serotonin | < 0.001 |
| 6-sulfatoxymelatonin | < 0.001 |
| N-acetylserotonin | 0.045 |
| 5-hydroxy-indole acetic acid | < 0.001 |
| 5-methoxytryptamine | 0.007 |
| 5-methoxytryptophane | < 0.001 |
| 2-methyl-5-hydroxytryptamine | < 0.001 |
| 5-methoxypsoralen | < 0.001 |
| 5-methoxytryptophol | 0.002 |
| chloramelatonin | 1.3 |
| caffeine | < 0.001 |
| caffeine acid | <0.001 |
| soluble coffee | <0.001 |
| soluble coffee decaffeinated | <0.001 |

Figure 3 Correlation EK-DSM / RK-DSM

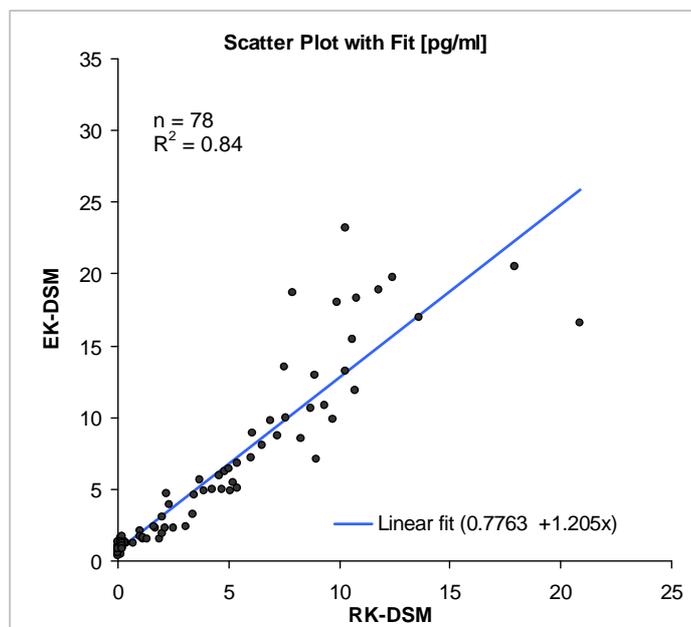


Table description: cf. "Results" and "Performance Characteristics" (page 4) and „Method Comparison“ (page 4).

APPENDIX II REFERENCES

1. Koorengel, KM, *et al.* A forced desynchrony study of circadian pacemaker characteristics in seasonal affective disorder. *J Biol Rhythms* **17**, 463-75 (2002).
2. Wirz-Justice, A, *et al.* No evidence for a phase delay in human circadian rhythms after a single morning melatonin administration. *J Pineal Res* **32**, 1-5 (2002).
3. Graw, P, *et al.* Early morning melatonin administration impairs psychomotor vigilance. *Behav Brain Res* **121**, 167-72 (2001).
4. Danilenko, KV, *et al.* Is sleep per se a Zeitgeber in humans. *J Biol Rhythms* **18**, 170-8 (2003).
5. Vaughan G M: New sensitive serum melatonin radioimmunoassay employing the Kennaway G280 antibody: Syrian hamster morning adrenergic response. *J Pineal Res* **15**, 88-103 (1993).
6. Voultsios, A, *et al.* Salivary melatonin as a circadian phase marker: validation and comparison to plasma melatonin. *J Biol Rhythms* **12**, 457-466 (1997)

**Direct Saliva Melatonin
Sample Pretreatment (Saliva)**

Clean polypropylene tube

200 µl Saliva Sample or Control
25 µl Pretreatment Solution



Vortex, 5 sec

Incubate, 10 min, 18-28°C

25 µl Neutralization Solution



Vortex, 5 sec

Centrifuge at 10'000 rpm for 5 min

Proceed to ELISA procedure

**Direct Saliva Melatonin
ELISA Procedure**

Precoated Microtiter Plate



Wash 2x

100 µl Calibrators, Pretreated Controls
or Samples



Incubate 16-20 hours at 2-8°C

add 50 µl Melatonin-Biotin-Conjugate



1 minute on a plate Rotator

3 hours at 2-8°C

Wash 4x

add 100 µl Enzyme Label



*60 minutes at 18-28°C
on a plate rotator*

Wash 4x

add 100 µl TMB Substrate



*Incubate 30 minutes at 18-28°C
on a plate rotator*

add 100 µl Stop Solution

➔ Read absorbance at 450 nm (within 30 minutes)

Salivette® is a registered Trademark from Sarstedt AG Nümbrecht, Germany

| Symbol | Explanation |
|---|-----------------------------------|
|  | Use By |
| REF | Catalogue number |
| LOT | Batch code |
|  | Contains sufficient for <n> tests |
|  | Consult Instructions for Use |
|  | Temperature limitation |
| REAG PRE | Pretreatment Reagent |
| SOLN NEUT | Neutralizing Solution |
| MP | Microtiterplate |

| Symbol | Explanation |
|----------------------|-------------------------------|
| BUF WASH 10X | Wash Buffer Concentrate (10x) |
| REAG BLANK | Blanking Reagent |
| BUF INC | Incubation Buffer |
| CAL A - CAL E | Calibrator A -E |
| CONTROL L | Control Low |
| CONTROL H | Control High |
| BC | Biotin Conjugate |
| EL | Enzyme Label |
| SUBS TMB | TMB Substrate |
| SOLN STOP | Stop Solution |