



anti-MAG Antibodies ELISA

MAG = Myelin Associated Glycoprotein

For research use only.
Not for use in diagnostic procedures.

EK-MAG-U 96 tests

Release Date: 2024-07-22
Version A3

 **Manufacturer**

BÜHLMANN Laboratories AG
Baselstrasse 55
4124 Schönenbuch, Switzerland
Tel.: +41 61 487 12 12
Fax: +41 61 487 12 34
info@buhlmannlabs.ch

INTENDED USE

The anti-MAG Antibodies ELISA is an assay for the semi-quantitative determination of anti-MAG IgM antibodies in human serum samples.

For research use only. Not intended for use in diagnostic procedures.

PRINCIPLE OF THE ASSAY

The anti-MAG Antibodies ELISA allows the measurement of IgM antibodies against the Myelin Associated Glycoprotein (MAG) in serum by sandwich ELISA. The microtiter plate is coated with purified MAG from human brain. Serum samples, controls, and calibrators are added to the wells of the microtiter plate. After 2 hours of incubation at 2 – 8°C and washing steps, a detection antibody conjugated to horseradish peroxidase (HRP) detects the anti-MAG antibodies bound to the human MAG on the plate. After another 2 hours of incubation and further washing steps, the chromogenic HRP substrate, tetramethylbenzidine (TMB), is added (blue color formation) followed by a stopping reaction (change to yellow color). The absorption is measured at 450 nm.

The level of anti-MAG antibodies is determined using the calibration curve generated from the measured calibrator values and is expressed as BÜHLMANN Titer Unit (BTU).

REAGENTS SUPPLIED AND PREPARATION

Reagents	Quantity	Code	Reconstitution
Microtiter Plate 96 wells precoated with human MAG	12 x 8-well strips with frame	B-MAG-MP	Ready to use
Plate Sealer	3 pieces		
Wash Buffer Concentrate (10x)	1 bottle x 100 mL	B-MAG-WB	Dilute with 900 mL of deionized water
Incubation Buffer with preservatives	1 bottle x 100 mL	B-MAG-IB	Ready to use
Calibrators A to D¹ lyophilized with preservatives	4 vials	B-MAG-CASET	Add 1 mL of Incubation Buffer
Low and High Control² lyophilized with preservatives	2 vials	B-MAG-CONSET	Add 1 mL of Incubation Buffer
Enzyme Label IgM Anti-human IgM antibody conjugated to HRP in a buffer matrix with preservatives	1 vial x 11 mL	B-MAG-ELM	Ready to use Blue solution
TMB Substrate TMB in Citrate buffer	1 vial x 11 mL	B-TMB	Ready to use
Stop Solution 0.25 M Sulfuric acid	1 vial x 11 mL	B-ST5	Ready to use Corrosive agent

Table 1

¹ After reconstitution, calibrators A, B, C and D contain 70000, 15000, 3000 and 1000 BÜHLMANN Titer Units (BTU) of anti-MAG antibodies, respectively.

STORAGE AND SHELF LIFE OF REAGENTS

Sealed / unopened Reagents	
Store at 2-8 °C. Do not use the reagents beyond the expiration date printed on the labels.	
Opened / reconstituted reagents	
Microtiter Plate	Return unused strips immediately to the foil pouch containing the desiccant packs and reseal along the entire edge of zip-seal. Store for up to 1 month at 2-8 °C.
Diluted Wash Buffer	Store for up to 1 month at 2-8 °C.
Incubation Buffer	
Enzyme Label IgM	
TMB Substrate	
Controls	Aliquot after reconstitution and store at ≤-20 °C. Store for up to 1 month at ≤-20 °C. ¹
Calibrators	
Stop Solution	Store for up to 1 month at 18-28 °C.

Table 2

¹ Reconstituted calibrators and controls can be subject to three freeze-thaw cycles during the 1 month.

MATERIALS REQUIRED BUT NOT PROVIDED

- Precision pipettes with disposable tips: 10 µL, 20 µL, 100 µL and 1000 µL pipettes
- Disposable polystyrene or polypropylene tubes for the preparation of sample dilutions
- 1000 mL cylinder for the dilution of the wash buffer
- Microtiter plate washer
- Blotting paper
- Microtiter plate shaker
- Microtiter plate reader for measurement of absorbance at 450 nm.

WARNINGS AND PRECAUTIONS

Safety precautions

- The calibrators, controls and microtiter plate of this kit contain components of human origin. Although tested and found negative for HBV, HCV and HIV1/2, the reagents should be handled as if capable of transmitting infections and should be handled in accordance with Good Laboratory Practices (GLP) using appropriate precautions.
- This kit contains components classified in accordance with the Regulation (EC) No. 1272/2008:
 - The stop solution contains sulfuric acid (conc. 2.5 – 5%), thus the reagents may cause skin irritation (H315), serious eye irritation (H319), and may be corrosive to metals (H290).
 - The calibrators, and controls contain gentamicin sulfate (powder), thus, the reagents may cause an allergic skin reaction (H317) and allergy or asthma symptoms or breathing difficulties if inhaled (H334). And they contain thiomersal (powder), thus, the reagent is fatal if swallowed, in contact with skin, or if inhaled (H300+H310+H330).
 - The incubation buffer and enzyme label contain gentamicin sulfate (conc. < 1%), thus, the reagents may cause an allergic skin reaction (H317).

- Avoid contact of reagents with the skin, eyes, or mucous membranes. If contact does occur, immediately wash with generous amounts of water; otherwise, irritation / burns can occur.
- Reagents and chemicals have to be treated as hazardous waste according to the national biohazard safety guideline or regulation.

Technical precautions

- Read the instructions carefully prior to carrying out the test. Test performance will be adversely affected, if reagents are incorrectly diluted, modified or stored under conditions other than those as detailed in this instruction for use.

ELISA procedure

Temperature of reagents

- Prepare reagents before starting the assay procedure. Steps 3-9: Reagents used in steps 3-9 must be cold (2-8 °C) and kept cold while pipetting and washing. Recommendation: Prepare the wash buffer the day before performing the assay and place it into the fridge overnight.
- Perform all wash steps with cold (2-8 °C) wash buffer.
- Adjust TMB substrate and stop solution to room temperature (18-28 °C) at the start of the assay procedure.

Washing steps

- Wash steps 3, 6 and 9 are crucial to remove residues resulted from the production process and/or potentially unbound antibodies in the wells.
- An automated washer operating in “plate mode” is strongly recommended, i.e. each process step (dispense / aspiration) is carried out on all of the strips, sequentially, before the instrument continues with the next washing cycle.
- Make sure that all wells are completely empty after the last washing cycle.

Substrate incubation

- Step 11: Shake the microtiter plates during incubation with substrate. Depending on the model of the plate shaker we recommend 400-600 rpm. The solution should move in the wells but must not spill over.

Additional sample dilution

- Samples exceeding 70'000 BTU can be diluted into the analytical measurement range (>1000 BTU, <70'000 BTU). Use incubation buffer for dilution of serum samples.

Kit components

- Components must not be used after the expiry date printed on the labels.
- Do not mix different lots of reagents.
- Every effort should be made to ensure that no cross contamination occurs between reagents, samples or between wells.
- Microwells cannot be re-used

SPECIMEN COLLECTION AND STORAGE

The procedure requires <0.1 mL of blood or <50 µL of serum, respectively.

Collect blood into plain venipuncture tubes without any additives and avoid hemolysis. Perform serum preparation according to manufacturer's instructions. Decant the serum.

Serum samples can be stored at 2-8 °C for up to 16 days or at -20 °C up to 12 months. Frozen samples should be thawed and mixed thoroughly by gentle swirling or inversion prior to use.

We recommend preparing aliquots of serum samples before freezing in order to avoid repeated freeze/thaw cycles.


ASSAY PROCEDURE

Note: Adjust TMB substrate solution to room temperature (18-28 °C).

1. Dilute samples 1:1000 with incubation buffer. Use e.g. 2 µL of serum + 2000 µL of cold! (2-8 °C) incubation buffer. Mix thoroughly by vortexing and leave diluted samples as well as reconstituted calibrators and controls at 2-8 °C for 30 minutes prior to pipetting (refer to steps 4a - c).
2. Prepare a plate-frame with sufficient strips to test the calibrators, controls and samples. Remove excess strips from the frame and reseal it in the foil pouch together with the desiccant packs without delay. Store refrigerated.


Note: Use cold reagents in steps 3 to 9.

3. Wash the wells four times using at least 300 µL of cold! (2-8 °C) wash buffer per well. Empty wells and tap plate firmly onto blotting paper to remove remaining liquid completely.

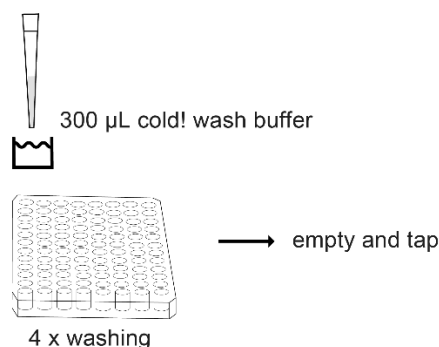


- 4a. Pipet 100 µL of incubation buffer (blank) in duplicate and Pipet 100 µL of calibrator A-D in duplicate into the respective wells.
- 4b. Pipet 100 µL of the controls low and high in duplicate into the respective wells.
- 4c. Pipet 100 µL of each diluted sample into the subsequent wells.
5. Cover the plate with a plate sealer and incubate for 2 hours (±5 min) at 2-8 °C (do not shake the plate).
6. Remove the plate sealer. Empty the wells and wash four times using at least 300 µL of cold! (2-8 °C) wash buffer per well. Empty the wells and tap the plate firmly


onto blotting paper in order to remove wash buffer completely.

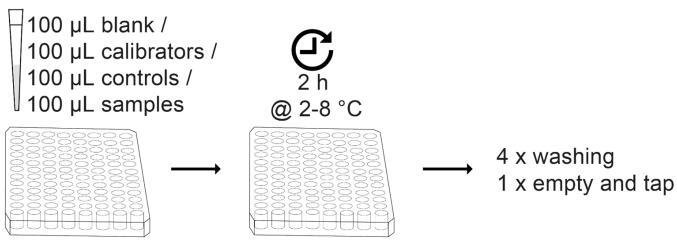


7. Add 100 µL of enzyme label IgM to all wells.
8. Cover the plate with a plate sealer and incubate for 2 hours (± 5 min) at 2-8 °C (do not shake the plate).
9. Remove the plate sealer. Empty the wells and wash four times using at least 300 µL of cold! (2-8 °C) wash buffer per well. Empty the wells and tap the plate firmly onto blotting paper.

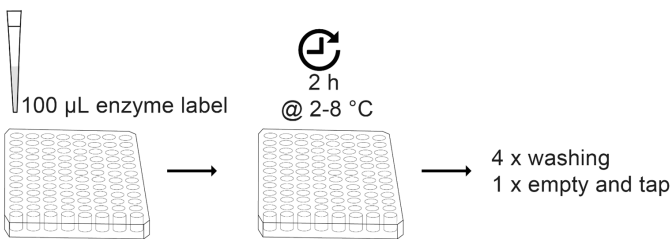

10. Add 100 µL of TMB substrate solution (equilibrated to room temperature) to each well.
11. Cover the plate with a plate sealer, protect the plate from light and incubate on a plate shaker set at 400-600 rpm, at 18-28 °C for 30 \pm 2 minutes.

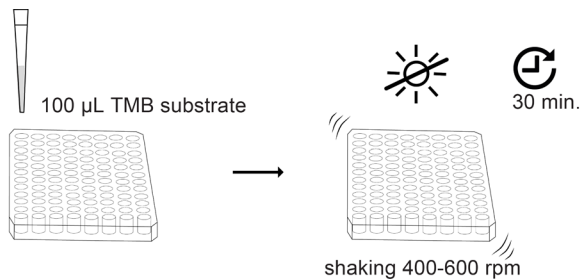

12. Add 100 µL of stop solution to all wells. Remove air bubbles with a pipette tip. Proceed to step 13 within 30 minutes.
13. Read the absorbance at 450 nm in a microtiter plate reader.

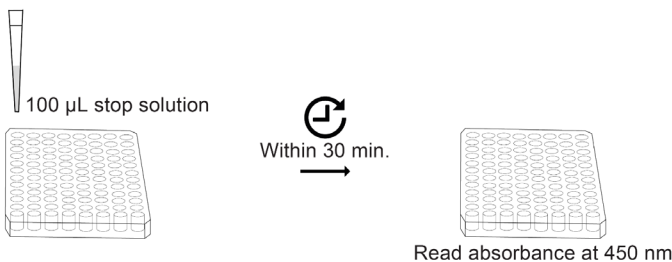

QUALITY CONTROL

Thorough understanding of this instruction for use is necessary for the successful use of the product. Reliable

results will be obtained only by using precise laboratory techniques and accurately following this instruction for use. The anti-MAG Antibodies ELISA kit comes with two controls: controls low and high. The controls have assigned value ranges indicated on the QC-data sheet supplied with each kit. The control measurements must be within the indicated value ranges to obtain valid results.

In addition to kit controls, we recommend the use of serum pools for internal quality control.

The reproducibility of standard curve parameters and control values should be within established limits of laboratory acceptability. If the performance of the assay does not meet the established limits and repetition has excluded errors in technique, check the following issues: i) temperature controlling (reagents used in step 3-9 kept at 2-8 °C) ii) accuracy of thermometers, pipetting and timing devices; iii) ELISA reader settings; iv) expiration dates of reagents; v) storage and incubation conditions; vi) color of TMB substrate solution (should be colorless); vii) purity of water; viii) aspiration and washing methods.

STANDARDIZATION AND METROLOGICAL TRACEABILITY

There are no internationally or nationally recognized reference materials or reference measurement procedures for anti-MAG antibodies in serum samples. The anti-MAG Antibodies ELISA is standardized against an internally established reference material. Calibrator and control values are assigned according to a value transfer protocol (ref. 1,2), to guarantee metrological traceability and are indicated in arbitrary BÜHLMANN Titer Units. The 95% confidence interval of the combined uncertainty of product calibrators and controls is lower than 35%.

CALCULATION OF TEST RESULTS

Standard curve

Use a software program capable of the following calculations:

- subtract the blank OD value from each calibrator well to calculate the calibrator value.
- Establish a standard curve using a 4-parameter logistic (4 PL) fit.

Controls and Samples

Use a software program capable of the following calculations;

- subtract the blank OD value from each control/ sample well. Calculate anti-MAG antibody level of the controls / sample in each well, in BTU, using the established standard curve.

Note: Results presented in table 4 and figure 1 are examples and are provided for demonstration purposes only. A calibration curve must be generated for each set of samples to be tested.

LIMITATIONS

- There is currently no internationally accepted reference method for the detection of anti-MAG IgM antibodies. Refer to the chapter "Standardization and metrological traceability".
- This test has not been validated for CSF, and plasmapheresis.

- Intravenous immunoglobulins (IVIg) and cryoglobulins may affect test results.

RESULT CATEGORIES

There are two result categories for the anti-MAG antibodies ELISA assay:

Result category	Presence of anti-MAG antibodies
< 1000 BTU	No
≥ 1000 BTU	Yes

Table 3

PERFORMANCE CHARACTERISTICS

Performance characteristics are based on mean results from 2 wells.

Repeatability: 3.2 – 11.8%

Within-laboratory precision: 5.5 – 15.9%

Repeatability and within-laboratory precision were established according to the CLSI guideline EP05-A3 using the standardized 20 days x 2 runs x 2 replicates study design. Four (4) pooled human serum samples, covering the measuring range of the assay, were tested.

A fifth sample at 213 BTU yielded 79/80 results (98.8%) within category (< 1'000 BTU). The results are summarized in table 5 and 6.

Reproducibility: 10.0 – 21.6% CV

Reproducibility was established according to the CLSI guideline EP05-A3 by performing measurements using a 3 operators x 3 instruments/lots x 5 days x 5 replicates study design. Four (4) pooled human serum samples, covering the measuring range of the assay, were tested. A fifth sample at 55 BTU yielded 75/75 results (100.0%) within category (< 1'000 BTU). The results are summarized in table 7 and 8.

Limit of Detection (LoD): 305 BTU

The LoD was established according to the CLSI guideline EP17-A2 using a non-parametric analysis with a proportion of false positive (α) less than 5% and false negative (β) less than 5% based on 120 determinations, with 60 blank and 60 low level replicates, and a **LoB of 138 BTU**.

High dose hook effect

Samples with anti-MAG antibody levels of up to 2.8×10^5 BTU can be measured without limiting the measuring range of the assay.

INTERFERING SUBSTANCES

The susceptibility of the Anti-MAG Antibodies ELISA assay to oral and injectable pharmaceuticals, as well as to endogenous substances was assessed according to the CLSI guideline EP07-A3. Bias in results exceeding 20% was considered interference.

No interference was detected with the following substances up to the listed concentrations: intravenous immunoglobulin (20 mg/mL), cladribine (273 ng/mL), Interferon alpha-2a (49.5 ng/mL), ibuprofen (0.22 mg/mL), rheumatoid factor (680 IU/mL), hemoglobin (10 mg/mL), hemolysate (10 mg/mL), triglyceride (20 mg/mL), conjugated bilirubin (0.4 mg/mL), unconjugated bilirubin (0.4 mg/mL).

TABLES AND FIGURES

Examples of results

	Level [BTU]	Absorbance [OD]	Calc. Level [BTU]	CV [%]
Blank 1		0.046		
Blank 2		0.049		
Average		0.048		
Calibrator A	70000	2.195	70497	
Calibrator A	70000	2.188	69508	
Average	70000	2.191	70000	0.2
Calibrator B	15000	1.272	15313	
Calibrator B	15000	1.245	14693	
Average	15000	1.258	15000	1.5
Calibrator C	3000	0.417	3070	
Calibrator C	3000	0.400	2931	
Average	3000	0.408	3000	2.9
Calibrator D	1000	0.135	1009	
Calibrator D	1000	0.132	991	
Average	1000	0.134	1000	1.5
Control LOW		0.360	2602	
Control LOW		0.376	2731	
Average		0.368	2666	3.1
Control HIGH		1.395	18433	
Control HIGH		1.383	18090	
Average		1.389	18261	0.6
Sample 1		0.001	255	
Sample 1		0.009	297	
Average		0.005	276	116.5
Sample 2		1.092	11599	
Sample 2		0.969	9511	
Average		1.030	10555	8.5

Table 4

Example of standard curve (OD₄₅₀)

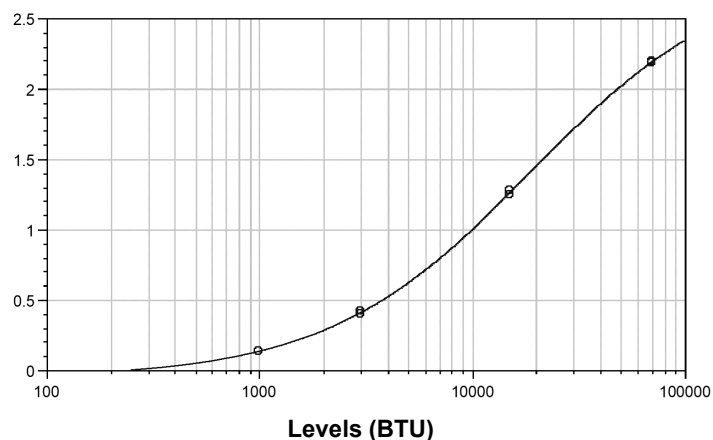


Figure 1

Within-laboratory precision

ID	Mean Level, BTU	n	Within-run		Between-run		Between-day		Within-laboratory	
			SD	%CV	SD	%CV	SD	%CV	SD	%CV
S2	2251	80	267	11.8	199	8.8	130	5.8	357	15.9
S3	8849	80	349	3.9	314	3.6	122	1.4	485	5.5
S4	19683	80	622	3.2	1492	7.6	908	4.6	1855	9.4
S5	37185	80	1684	4.5	3083	8.3	1466	3.9	3806	10.2

Table 5

ID	Description	n	Mean Level, BTU	% Within category
S1	< 1'000 BTU	80	213	97.5

Table 6

Reproducibility

ID	Mean Level, BTU	n	Within-run		Between-run		Between-day		Within-laboratory	
			SD	%CV	SD	%CV	SD	%CV	SD	%CV
S2	2802	75	181	6.5	517	18.4	261	9.3	606	21.6
S3	9052	75	258	2.9	821	9.1	279	3.1	904	10.0
S4	18241	75	531	2.9	1146	6.3	1475	8.1	1942	10.6
S5	34713	75	893	2.6	2740	7.9	2023	5.8	3521	10.1

Table 7

ID	Description	n	Mean Level, BTU	% Within category
S1	< 1'000 BTU	75	55	100.0

Table 8

Samples / Controls / Calibrators Preparation

Dilute serum samples 1:1000 with (cold)! incubation buffer and mix thoroughly by vortexing

Reconstitute or thaw (aliquoted) reconstituted controls and calibrators

leave 30 minutes at 2-8 °C

anti-MAG Antibodies ELISA

Precoated microtiter plate

wash 4 x with $\geq 300 \mu\text{L}$ (cold)! wash buffer

100 μL incubation buffer, calibrators, controls or serum samples (1:1000)

incubate 2 hours (± 5 min) at 2-8 °C

wash 4 x with $\geq 300 \mu\text{L}$ (cold)! wash buffer

add 100 μL enzyme label

incubate 2 hours (± 5 min) at 2-8 °C

wash 4 x with $\geq 300 \mu\text{L}$ (cold)! wash buffer

add 100 μL TMB substrate

incubate 30 minutes (± 2 min) at 18-28 °C on a plate shaker ~400-600 rpm

add 100 μL stop solution

Read absorbance at 450 nm (within 30 minutes)

TIME TO RESULT: 5 HOURS

REFERENCES

1. Blirup-Jensen, S., Johnson, A. M. & Larsen, M. Protein standardization V: Value transfer. A practical protocol for the assignment of serum protein values from a Reference Material to a Target Material. *Clin. Chem. Lab. Med.* **46**, 1470–1479 (2008);
2. CLSI guidelines EP30-A - Characterization and Qualification of Commutable Reference Materials for Laboratory Medicine (2010).

CHANGELOG

Date	Version	Change
2024-07-22	A3	IFU changes due to removal of Triton™ X-100 in some of the kit components: <ul style="list-style-type: none">- Update to in-use stabilities of reagents in chapter <i>Storage and shelf life of reagents</i>- Removal of precautionary notes regarding Triton™ X-100 in chapter <i>Warnings and Precautions</i>- Revision of sub-chapter <i>Limit of Detection</i> in chapter <i>Performance characteristics</i> Revision of <i>Short protocol</i> and chapter <i>Symbols</i>

SHIPPING DAMAGE

Please notify your distributor, if this product was received damaged.

SYMBOLS

BÜHLMANN use symbols and signs listed and described in ISO 15223-1.

For definition of symbols see the symbol glossary at: www.buhmannlabs.ch/support/downloads/

In addition, the following symbols and signs are used:

Symbol	Explanation
MP	Microtiter Plate
BUF INC	Incubation Buffer
BUF WASH 10X	Wash Buffer Concentrate (10x)
CONTROL L	Control Low
CONTROL H	Control High
CAL A - CAL D	Calibrator A - D
EL IgM	Enzyme Label IgM
SUBS TMB	TMB Substrate
SOLN STOP	Stop Solution